

# Supplementary Material for FACMIC: Federated Adaptive Clips for Medical Image Classification


Yihang Wu<sup>1</sup>, Christian Desrosiers<sup>2</sup>, and Ahmad Chaddad<sup>1,2</sup>

<sup>1</sup> Laboratory for Artificial Intelligence for Personalised Medicine, School of Artificial Intelligence, Guilin University of Electronic Technology, China


<sup>2</sup> Laboratory for Imagery Vision and Artificial Intelligence, ÉTS Montreal, Canada  
 ahmad8chaddad@gmail.com

**Table S1:** Implementation details of other comparative methods.

Methods	Details
FedProx	$\mu_{Prox} = 1e - 2/2$
MOON	$\mu_{MOON} = 1$
FedFocal	$\gamma = 1$

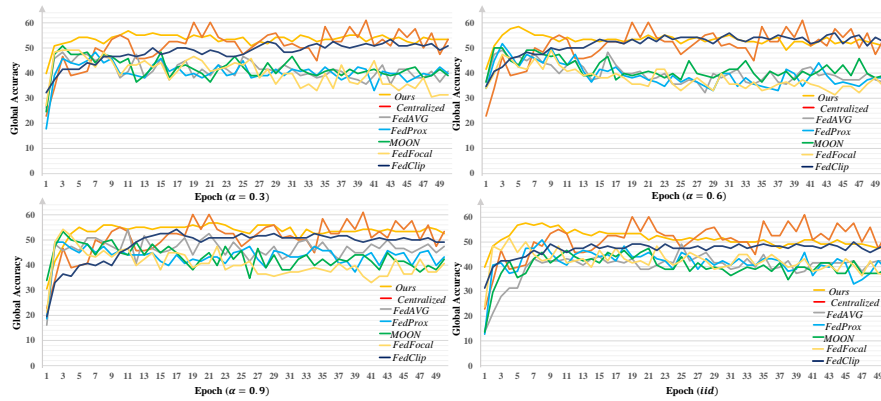

**Fig. S1:** Global testing ACC (%) using SC dataset for each round using our method and other comparable techniques.

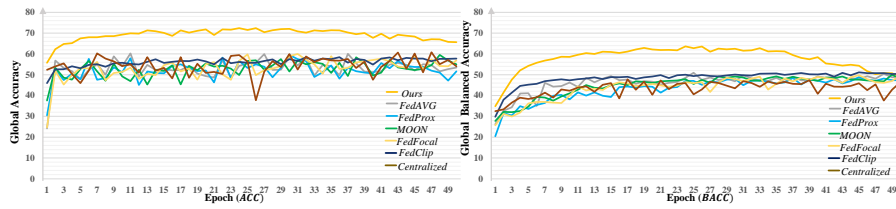

**Fig. S2:** Global testing accuracy (ACC%) and balanced accuracy (BACC%) using Real dataset for each round using our method and other comparable techniques.